

Application No.: 09/877,645
Applicant : CABEDO-DESLIERRES et al.
Examiner : Shay L. Balsis
Art Unit : 1744

c) Amendment to the Drawings

Following the informalities found by the Examiner and mentioned in pages 2 and 3 of the Office Action Summary, the Applicants - without adding any new matter - had to correct some of the Drawings, as follows:

On FIG. 1, FIG. 2, FIG. 3 - No corrections were incorporated .

On FIG. 3A - Minor corrections were incorporated for clarification of detail.

On FIG. 4, FIG. 5, FIG. 6, FIG. 7, FIG. 8, FIG. 9 , FIG. 10 - No corrections were incorporated.

On FIG. 10A - Previous part #20 is now corrected to #34.

On FIG. 11, FIG. 13 - No corrections were incorporated.

On FIG. 12 - Removed unnecessary callout #38 .

On FIG. 14 - Previous part #42 is now corrected to #41 , and minor correction incorporated in this part #41 for clarification of detail.

On FIG. 15 - Added omitted part #55 (in two places) and previous part #37 is now corrected to #44 (in two places).

We are enclosing a LIST OF PART NUMBERS.

Respectfully submitted,



Maria R. Cabedo-Deslierres

Application No.: 09/877,645

Applicant : CABEDO-DESLIERRES et al.

Examiner : Shay L. Balsis

Art Unit : 1744

LIST OF PART NUMBERS

- | | |
|--------------------------------------|-------------------------------------|
| 19 - Toothbrush Body | 46 - Threaded Shaft |
| 20 - Toothbrush | 47 - Close-out Cap |
| 21 - Handle | 48 - Serations |
| 22 - Brush | 49 - Recess Chamber |
| 23 - Bristles | 50 - Optional Toothbrush Embodiment |
| 24 - Neck of the Toothbrush | 51 - Handle |
| 25 - Recess Pocket | 52 - Forward Chamber |
| 26 - Button | 53 - Aft Chamber |
| 27 - Long Extension Tube | 54 - Center Chamber |
| 28 - Interdental Hard Brush | 55 - Structural Members |
| 29 - Recess Chamber | |
| 30 - Gum Massager and Stimulator Tip | |
| 31 - Slot | |
| 32 - Hollow Cylinders | |
| 33 - Axis | |
| 34 - Slider | |
| 35 - Slit | |
| 36 - Key | |
| 37 - Sliding Extension Tube | |
| 38 - Stem | |
| 39 - Hole | |
| 40 - Sliding Cover | |
| 41 - Tubular Support Arm | |
| 42 - Cross Member | |
| 43 - Projecting Pins | |
| 44 - Extension Tube | |
| 45 - Threaded Sleeves | |

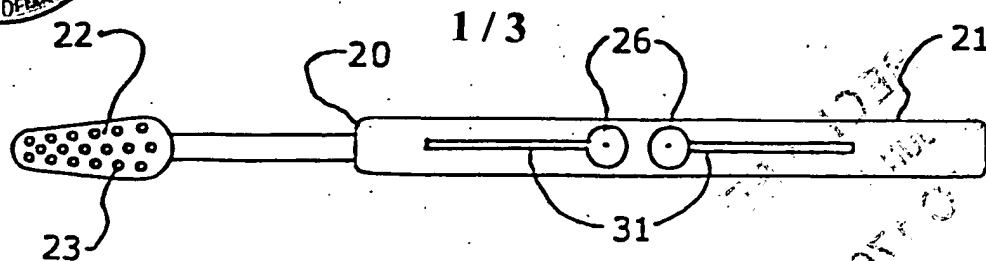




Fig. 1

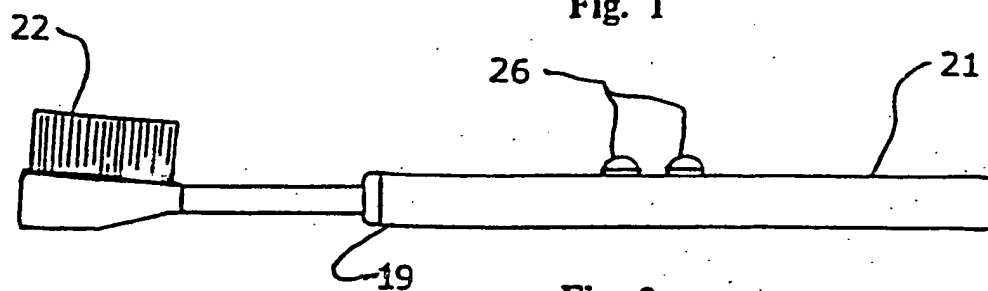


Fig. 2

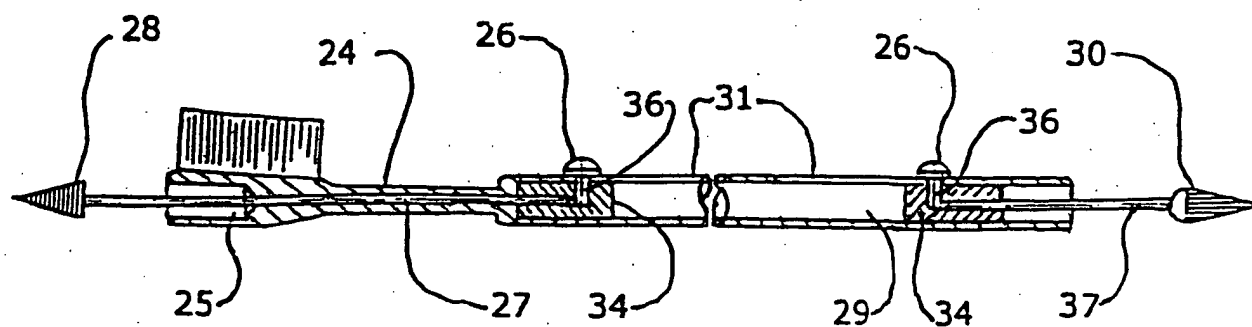


Fig. 3

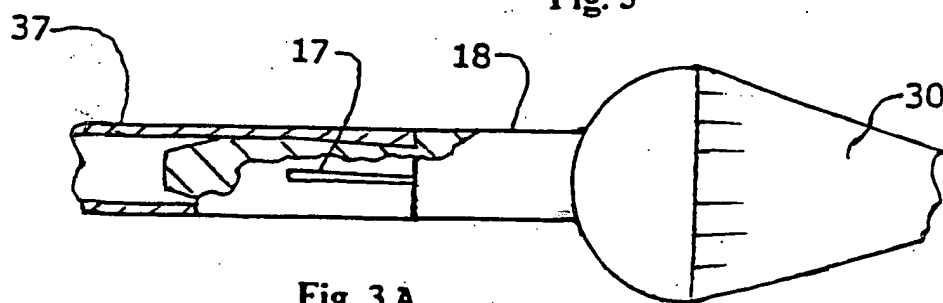


Fig. 3 A


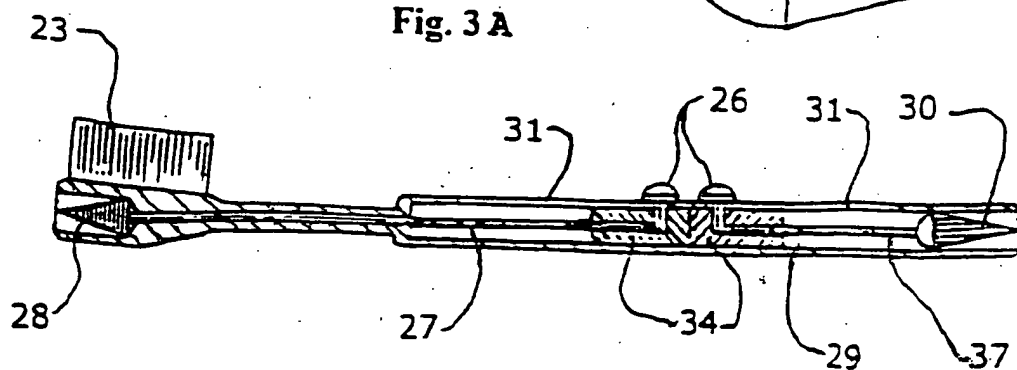


Fig. 4

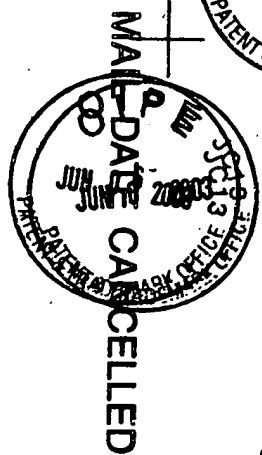

2 / 3

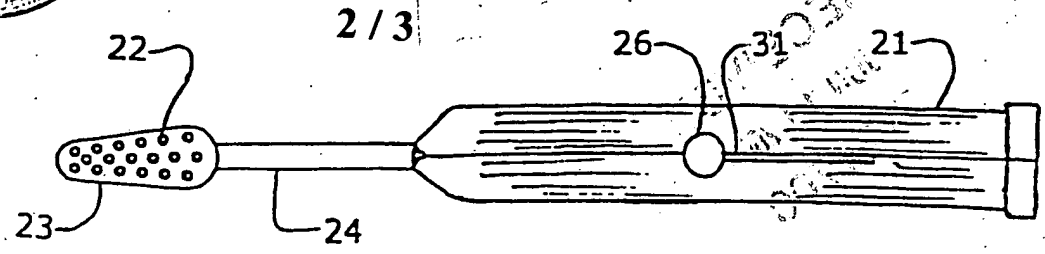


Fig. 5

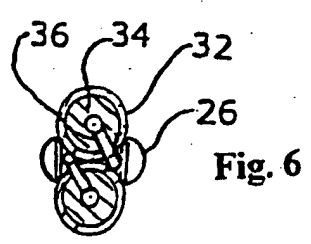


Fig. 6

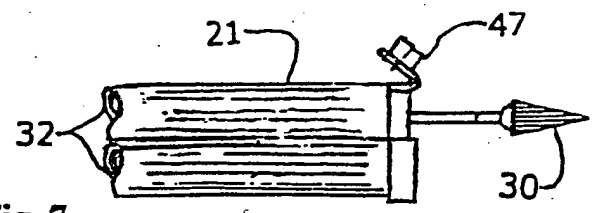


Fig. 7

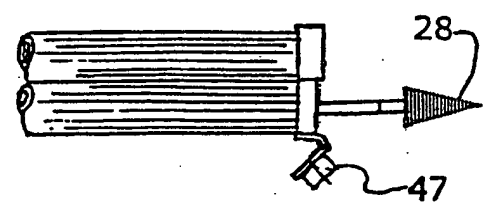


Fig. 8

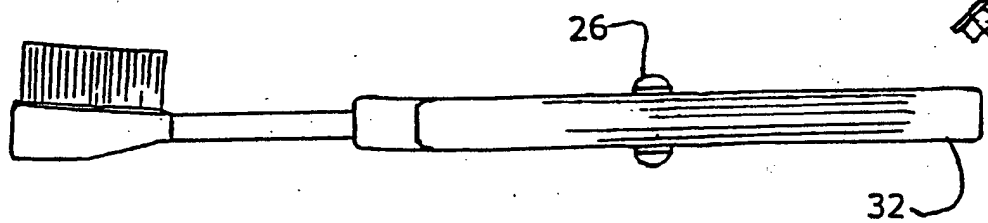


Fig. 9

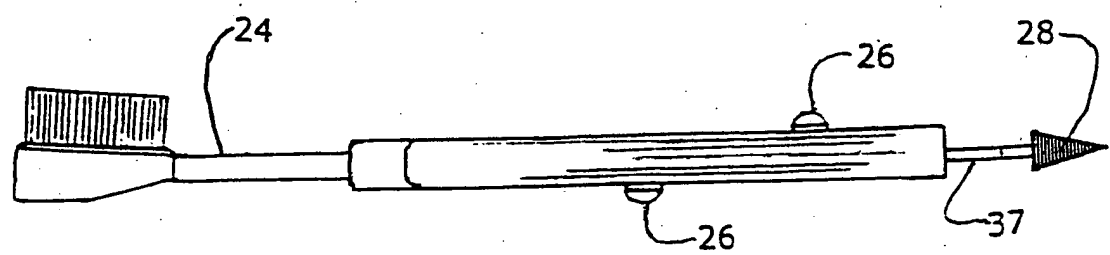


Fig. 10 A

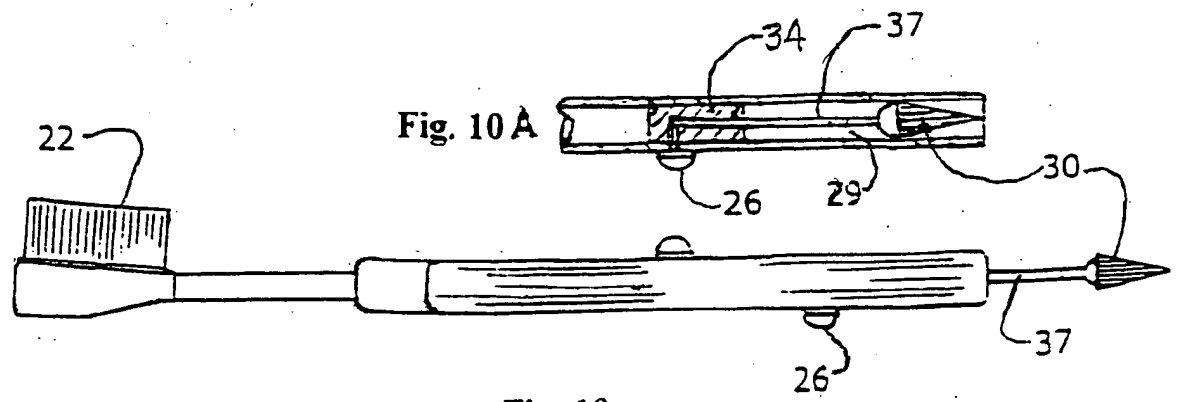


Fig. 10



3 / 3

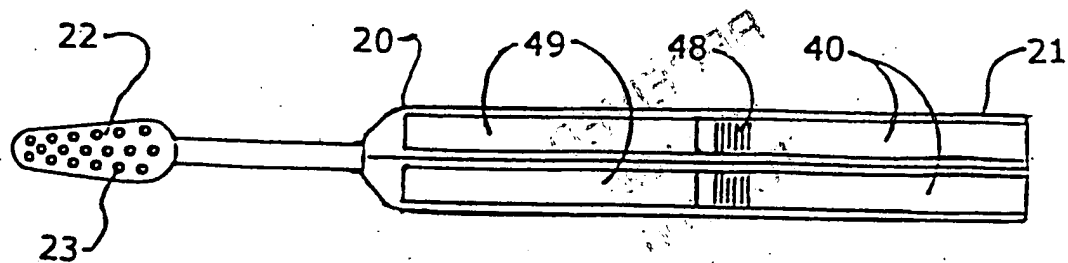


Fig. 11

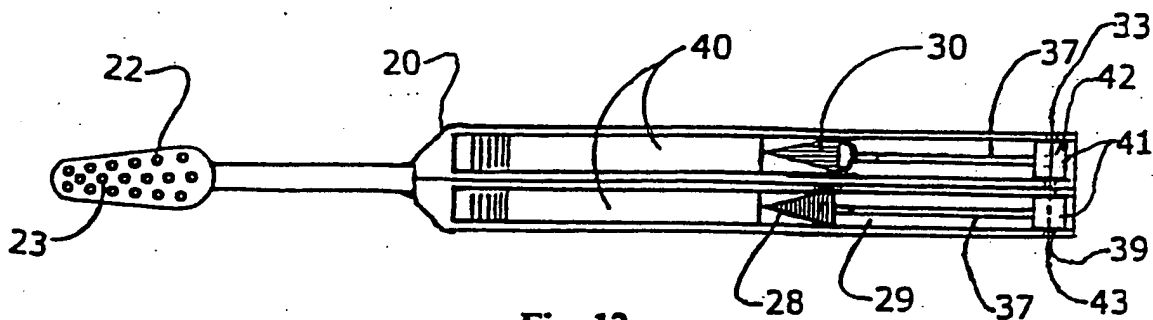


Fig. 12

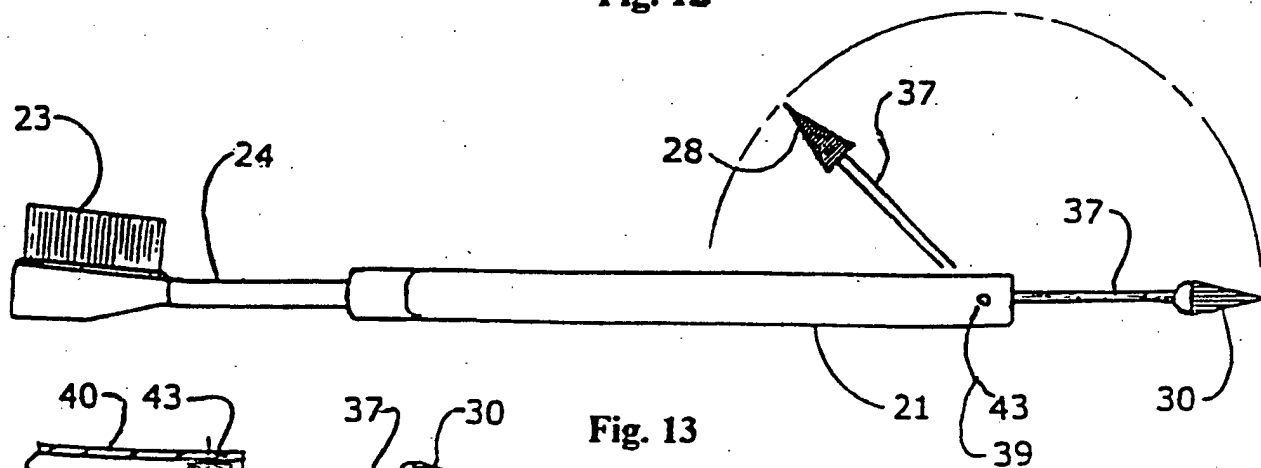


Fig. 13

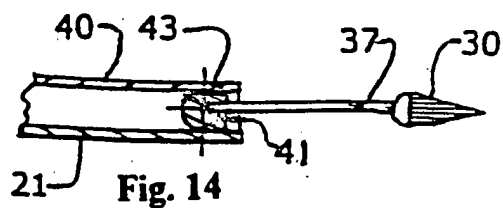


Fig. 14

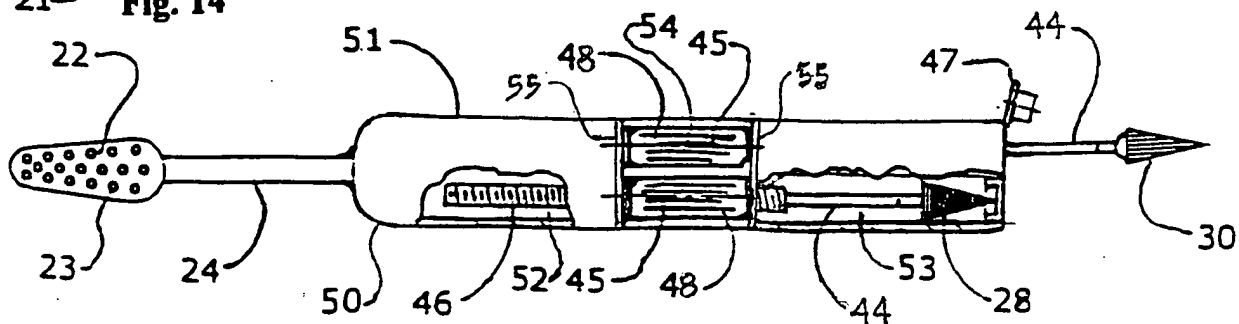


Fig. 15

Application No.: 09/877,645
Applicants : CABEDO-DESLIERRES et al
Examiner : Shay L. Balsis
Art Unit : 1744

RECEIVED
JUN 11 2003
TC 1700



AMENDMENT

d) Remarks

Upon receipt of the Official Action on the above Invention, the Applicants went through and revised all the items relating to the present Application, and verified that some incorrections needed amendment in order to avoid rejection. To speed up the process, - it was filed exactly two years ago, on 06/09/2001 - the Applicants decided not to wait for the Official Action that would point out such informalities but, instead, to proceed immediately to the necessary corrections in compliance with revised 37 CFR 1.121 .

Considering all the corrections that had to be produced and that a LIST OF PART NUMBERS was previously missing and is now attached hereto, the page numbers relating to the whole set of documents pertaining to this Patent Application were altered. Please take this fact into consideration.

Respectfully submitted,

Maria R. Cabedo-Deslierres